


VistaBrite Dimensions




Utility Water
Treatment System
for Instrument Washers

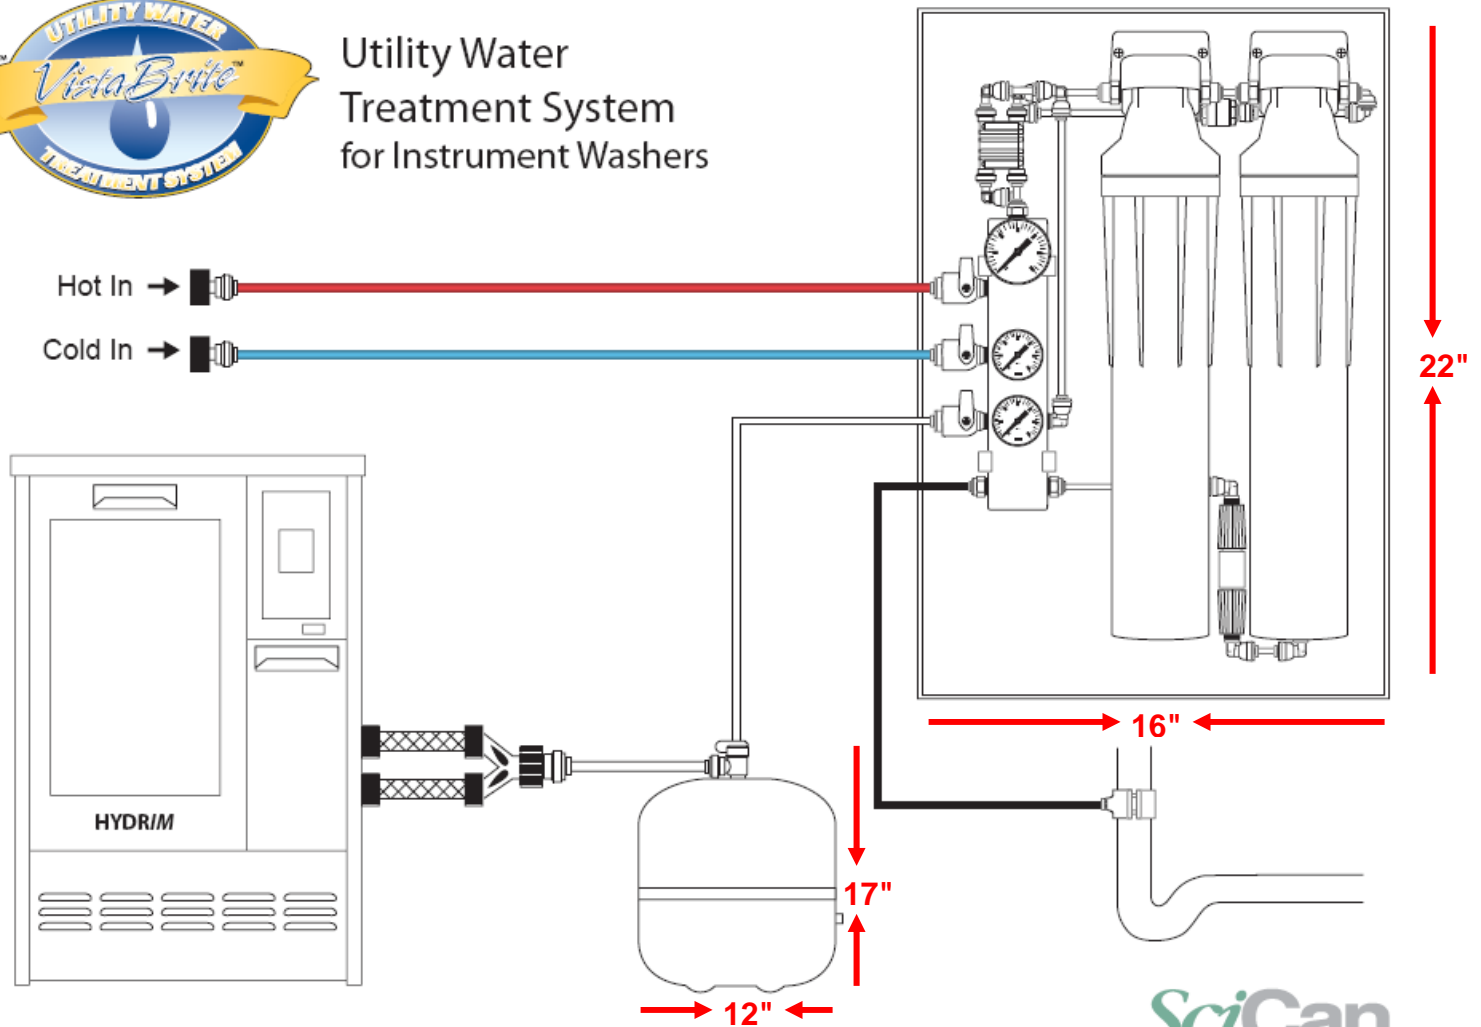


Typical Installation

SciCan

A HIGHER STANDARD

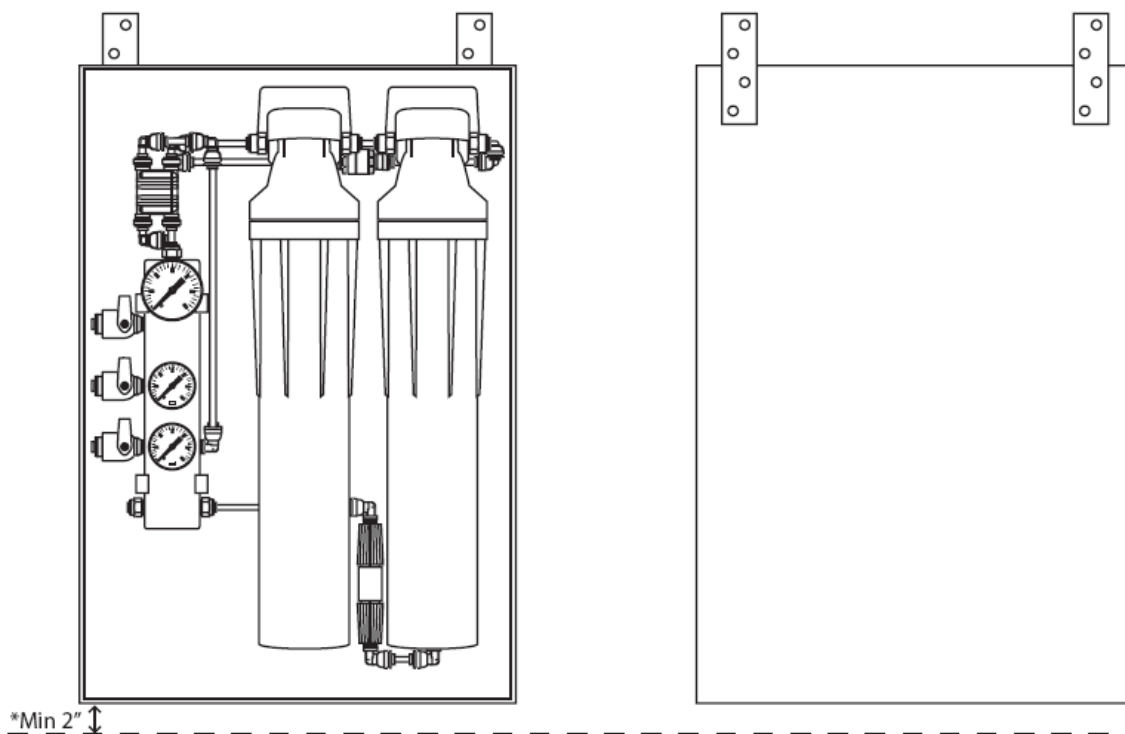

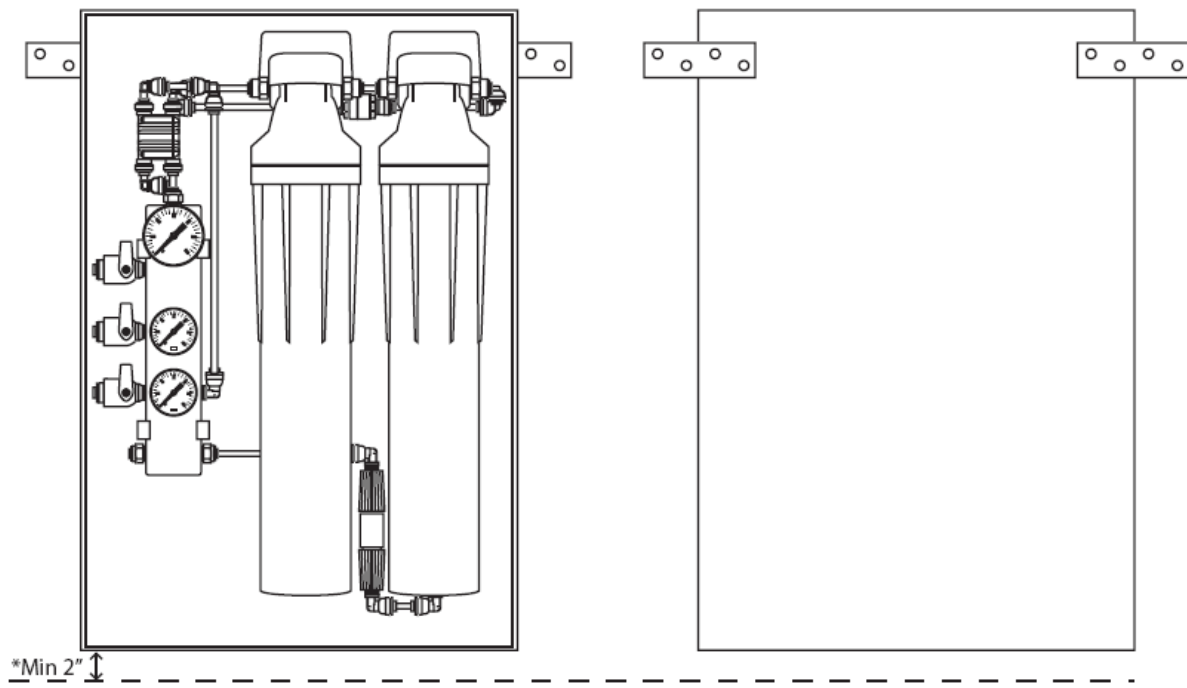

Mount units with at least 2" clearance at bottom to allow filter element replacement